



Audit 15

Out-of-trend (OOT) result

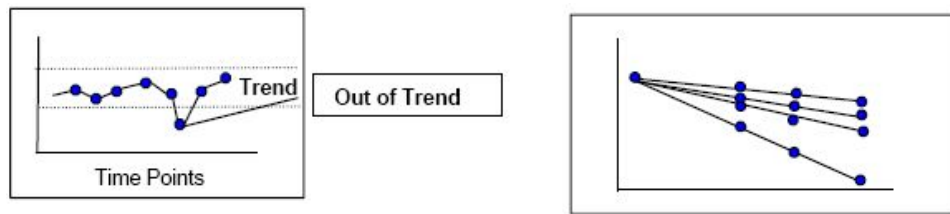

Precision and accuracy

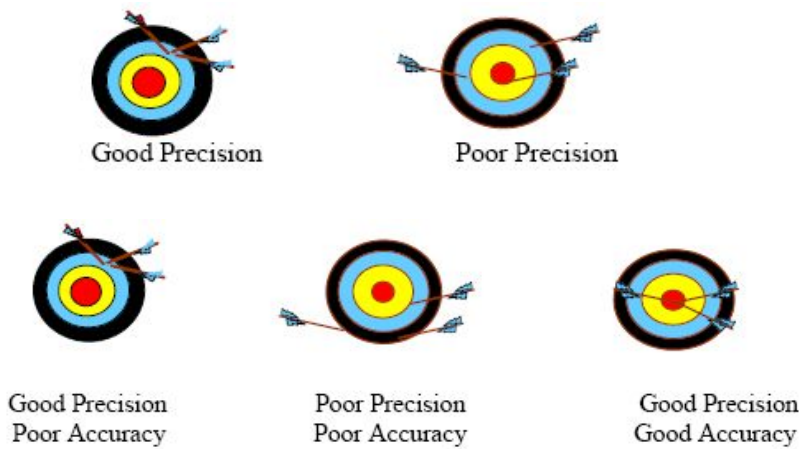


Methods


High Pressure Liquid Chromatography (HPLC)




HPLC Instrument

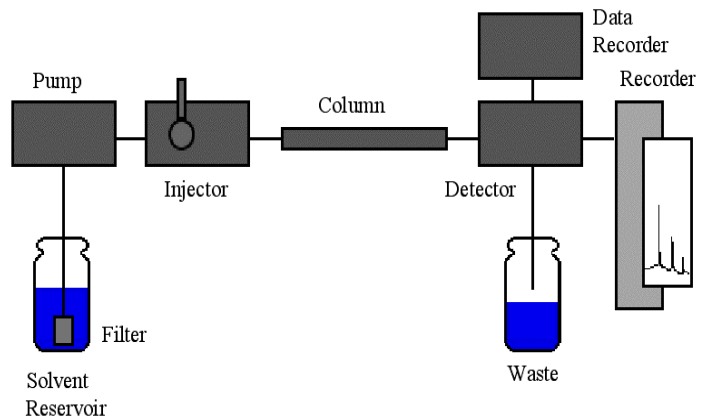

HPLC Chromatogram

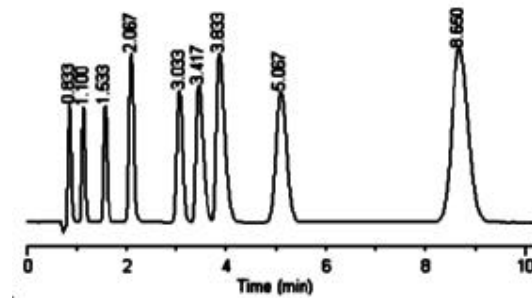


Gas chromatography

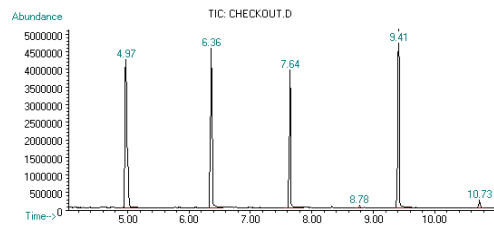


Gas chromatogram

Infrared spectroscopy


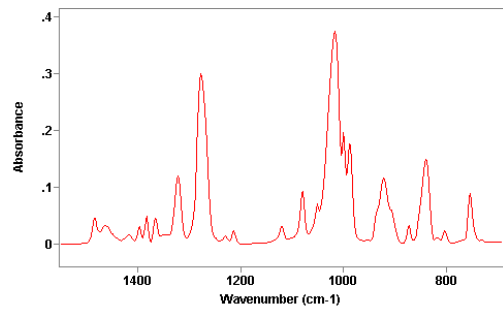


FTIR Spectrum

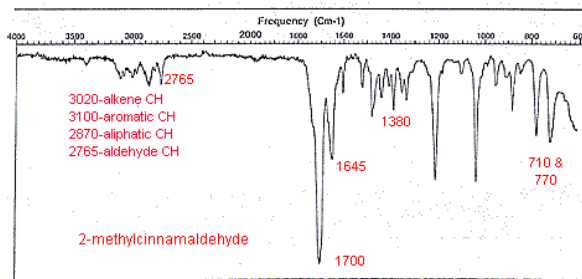

FTIR Spectrum

Mass spectrometer

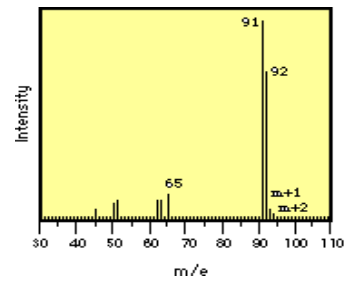

Dissolution Apparatus

